



## Electromedicals

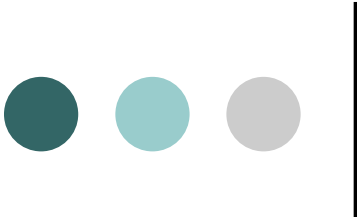

# Central Monitoring System

Upgradable to  
NiBP & Spo2

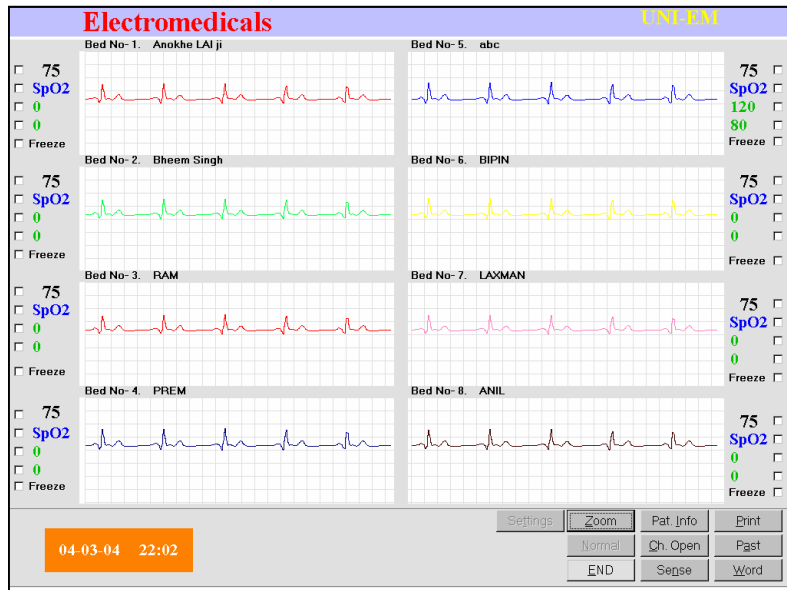

No. Of Beds:	Eight
Trace Duration:	4 Sec at 25mm/s Sweep Speed or 8 Sec for Max. 4 Beds at a time
Alarms	Upper Limit and Lower limit for the parameters purchased.
Input Data	Patient Details with daily report
Detection:	Arrhythmia detection
Trend	Trend for 24 Hrs for HR and all Arrhythmia Detected. 24 Hrs.
Memory	One Trace at a time
Zoom	Separate ectopic counter for each bed
Counter	Trace , Patient Name with Ectopic Counter and Bed No.
Display:	NiBP , Spo2 , EtCo2 , IBP and Transmitter , Receiver
Upgradeable to :	

### Electromedicals

Plot No:116,117 & 126,127  
Electronics Complex,  
Pardesipura  
Indore , M.P.

Phone: )7310230035 , 36  
Fax:+91-731-571406  
Email: Electromedicals@vsnl.net

*To get to the heart of matter accurately*